

PRODUCT DATA

Hand-held Reverberation Time Analyzer — Type 2250-F with Reverberation Time Software BZ-7227 and Qualifier Light Type 7831

Reverberation Time Software BZ-7227 extends the “Easy, Safe and Clever” mantra of Hand-held Analyzer Type 2250 to include Reverberation Time (RT) measurements.

Press the Start/Pause pushbutton, clap your hands – that is all it takes to do a basic measurement. The “traffic light” shows measurement status at a glance, and the resulting RT spectrum is shown as well as the average RT for the room.

Keep track of measurement positions in the colour map display, check the “smiley” indicators for measurement quality, and add spoken or text comments to positions or projects.

Measurements comply with the relevant parts of ISO standards including ISO 140, ISO 3382, and ISO 354.

Type 2250 is the innovative 4th generation hand-held analyzer from Brüel & Kjær. It comes fully equipped as a sound level meter with PC software for data transfer, archiving and export (see [Product Data BP2025](#) for more information).



Uses and Features

Uses

- Workplace acoustics
- Acoustics in auditoria, halls, public spaces, etc
- Building acoustics room correction
- Sound power room correction
- Absorption coefficient

Features (Type 2250-F)

- Hand-held reverberation time analysis
- Wide dynamic range – no range switching
- 1/3 or 1/1-octaves
- Impulse (Schroeder) Method
- Interrupted Noise Method

- Parallel or serial measurements
- Built-in pink and white noise generator
- Measurement position management
- Measurement quality indicators
- Voice or text annotations
- Displays RT spectrum, decay and ensemble average decay
- Calculates wide band average reverberation time
- PC software available for post-processing and reporting

Features (Type 7831)


- Calculates reverberation time
- Edits measurement results, including manual input of data
- Documentation and reporting facilities

Reverberation Time Defined

RT is the most important parameter describing the acoustic quality of a room or space. It is important for sound levels, speech intelligibility and the perception of music. In addition, it is used to correct for the effects of RT on building acoustics and sound power measurements.

RT is the decay time for sound in a room after the excitation stops. It is the time for a 60 dB drop in level, but the decay is usually measured over a 10, 20 or 30 dB drop and then extrapolated to the 60 dB range, see Fig. 1.

Fig. 1
Reverberation Decay Curve and Reverberation Time

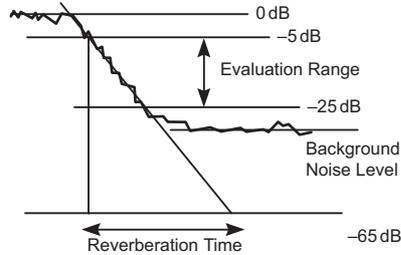


RT may be labelled EDT, T20 and T30 respectively for those three evaluation ranges. EDT is used in room acoustics only, while T20 and T30 may be used in all applications. RT is measured in 1/1- or 1/3-octave frequency bands, some of which may be averaged to provide a single-number result for the most significant bands.

RT may range from 0.1 seconds (or less) in anechoic chambers, to 10 or more seconds in large public spaces.


060191

Fig. 2
Typical displays from a Type 2250-F running RT software: the left-hand display shows how sources and receivers are mapped; the right-hand display shows an example of a receiver position table

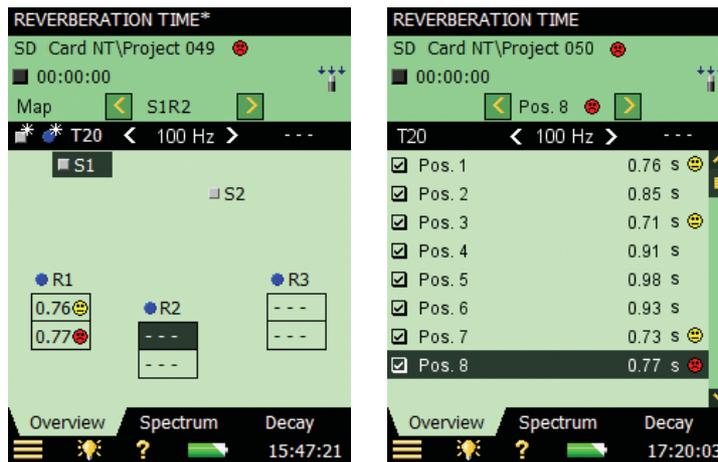

RT varies between positions in a room, so it is usually measured at several positions. The average for all positions gives an overall assessment, and the position results may be used to indicate the acoustic quality as a function of location, see the example displays in Fig. 2.

Fig. 3
Typical displays from a Type 2250-F running RT software: the left-hand display shows a Reverberation Time spectrum; the right-hand display shows a Reverberation Decay display

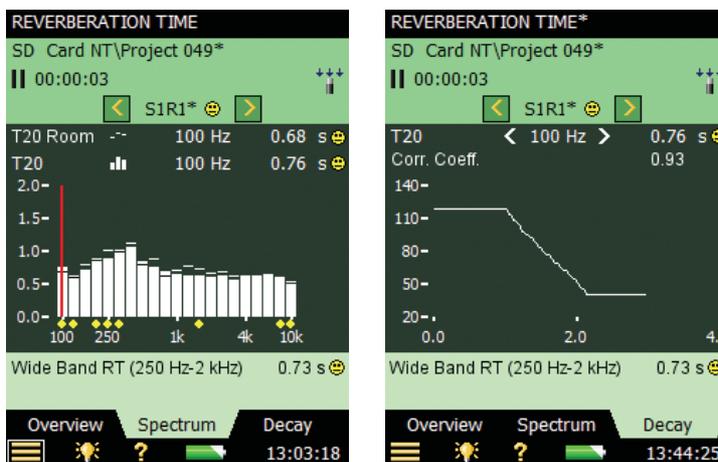

The average can be made for the RT spectra, or the decays for each frequency band may be averaged and the RT spectrum calculated for the averaged decays (ensemble average).

How Do We Measure Reverberation Time?

RT can be measured using either Impulsive Excitation (Schroeder Method), such as from a pistol or balloon burst (see Fig. 4), or by using Interrupted Noise with the built-in noise generator (see Fig. 5).

Impulsive Excitation Method

Fig. 4
Reverberation Time in the blink of an eye!




With Impulsive Excitation, all you need to carry is Type 2250-F, a tripod and a balloon (or other impulsive source, such as a starting pistol). After you pop the balloon, Type 2250-F will start measuring, analyse the decay and present the RT as well as the decay curves for all frequency bands.

It will also display the average RT for the bands you select.

The single input range means that trial measurements are not necessary when using the impulsive excitation method.

Interrupted Noise Method

Fig. 5
Typical measurement setup using a loudspeaker source

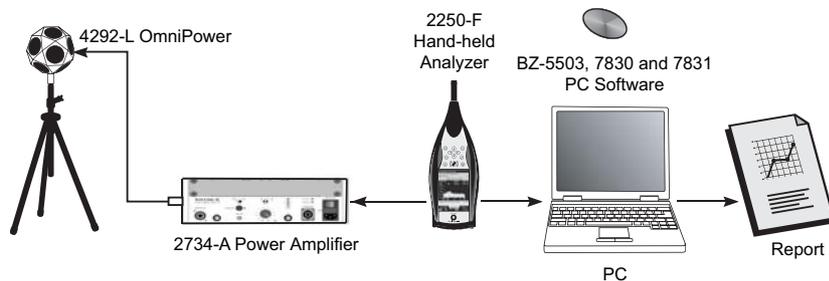


When using a power amplifier and loudspeaker sound source, Type 2250-F/BZ-7227 will turn its noise generator on and off, then measure and display the RT spectrum and decays.

The measurement can be in octaves or 1/3-octaves in parallel over a selectable frequency range, allowing you to focus sound power on the relevant range. In each frequency band, the decay is sampled 200 times each second, for reverberation times as long as 30 seconds. An example of a reverberation display is provided in Fig. 3.

The single input range speeds up the interrupted noise measurements by avoiding autorange.

Fig. 6
Typical display, with quality indicators

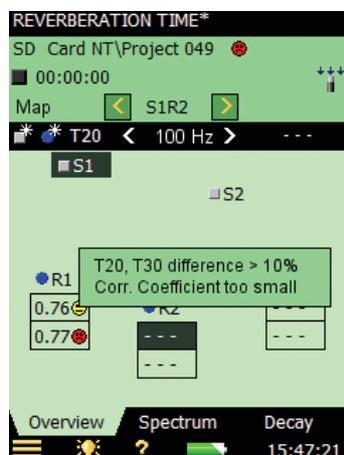

Measurement Displays

RT is shown as T20, T30 and EDT, and as decay curves with slope line and evaluation range. The room average RT is based on T20, T30 and EDT, or on the average decay for all positions (ensemble average).

Display Quality Indicators

To ensure user confidence, display quality indicators are provided in the form of 'smileys' on the display. If you tap on a smiley, the relevant details are displayed in a pop-up (see Fig. 6).

Status Codes

In addition, status codes are provided, which are saved with each measurement.

Accessories

A wide range of accessories including power amplifier, sound sources, and wireless transmission kit is available. And, of course, PC software for post-processing and reporting.

Who Should Use Reverberation Time Software?

The software has been designed specifically for use by professionals in the following industries:

- Occupational health officers assessing noise levels at workplaces. RT is often a contributing cause of high noise levels
- Environmental officers or consultants assessing sound insulation in new or renovated buildings. RT is one of the parameters for this assessment
- Consultants or acousticians assessing room acoustics in classrooms, auditoria, workspaces and public spaces
- Manufacturers or consultants estimating the sound power level for CE-labelling of tools or machinery, using RT for room correction

Where Can Reverberation Time Be Used?

RT software can be used in a variety of different applications:

Room Acoustics

RT is used in its own right for assessing the acoustics of workplaces, classrooms, auditoria, concert halls and public venues – to check or troubleshoot acoustical comfort or workplace health issues.

Building Acoustics

Sound levels measured in a receiving room are affected by the absorption in the room, by measuring RT you can correct level measurements for the absorption.

Sound Power Measurement

Tools, appliances and machinery must be CE-labelled with their sound power level. RT is part of a sound pressure based power measurement, made in a test room. RT is used to correct for the absorption of the test room.

Absorption Coefficient

RT is used to determine the absorption coefficient of building materials or building elements. In a specially designed reverberation chamber the RT is measured with and without a sample of material or building element. From this data the absorption coefficient (α) is calculated. The absorption coefficient is the ratio of reflected to incident sound energy. It is 1 for a totally absorbing material, and 0 for a totally reflecting material.

PC Software

Hand-held Analyzer Type 2250 comes with Measurement Partner Suite BZ-5503. It will control Type 2250 from a PC, manage and archive your measurement data, and keep your Type 2250 software up to date.

For analysing and reporting RT data, you can export your data from the BZ-5503 archive to Qualifier Light Type 7831 for viewing, editing and reporting.

For building acoustic applications (sound insulation), you need to measure RT *and* the source room/ receiving room levels, using Frequency Analysis Software BZ-7223. Then you can export your data from the BZ-5503 archive to Qualifier Type 7830 for viewing, editing, calculating sound insulation and reporting.

Note that Type 7831 and Type 7830 both include licenses for Noise Explorer™ Type 7815.

Hand-held Analyzer Type 2250 – Compliance with Standards

	CE-mark indicates compliance with: EMC Directive and Low Voltage Directive. C-Tick mark indicates compliance with the EMC requirements of Australia and New Zealand.
Safety	EN/IEC 61010–1: Safety requirements for electrical equipment for measurement, control and laboratory use. ANSI/UL 61010–1: Safety requirements for electrical equipment for measurement, control and laboratory use.
EMC Emission	EN/IEC 61000–6–3: Generic emission standard for residential, commercial and light industrial environments. EN/IEC 61000–6–4: Generic emission standard for industrial environments. CISPR 22: Radio disturbance characteristics of information technology equipment. Class B Limits. FCC Rules, Part 15: Complies with the limits for a Class B digital device.
EMC Immunity	EN/IEC 61000–6–1: Generic standards – Immunity for residential, commercial and light industrial environments. EN/IEC 61000–6–2: Generic standards – Immunity for industrial environments. Note 1: The above is guaranteed using accessories listed in this Product Data sheet only. Note 2: The above is guaranteed only when the AC output is not in use.

Specifications – Reverberation Time Software BZ-7227

The specifications given below are in addition to those for the [Type 2250 platform](#)

Standards

Conforms with the relevant parts of the following:

- IEC 61672–1 (2002–05) Class 1
- IEC 60651 (1979) plus Amendment 1 (1993–02) and Amendment 2 (2000–10), Type 1
- ANSI S1.4–1983 plus ANSI S1.4A–1985 Amendment, Type 1
- IEC 61260 (1995–07) plus Amendment 1 (2001–09), 1/1-octave bands and 1/3-octave bands, Class 0
- ANSI S1.11–1986, 1/1-octave bands and 1/3-octave bands, Order 3, Type 0–C
- ANSI S1.11–2004, 1/1-octave Bands and 1/3-octave bands, Class 0
- ISO 140
- ISO 3382
- ISO 354

CORRECTION FILTERS

For Microphone Types 4189, 4190, 4191, 4193, 4950, 4952 and 4184-A – BZ-7227 is able to correct the frequency response to compensate for sound field and accessories:

Broadband Measurements

DETECTORS

A- and C-weighted broadband detectors with F exponential time weighting

Overload Detector: Monitors the overload outputs of all the frequency weighted channels

MEASUREMENTS

L_{AF} and L_{CF} for display as numbers or quasi-analog bars

MEASURING RANGES

When using Microphone Type 4189:

Dynamic Range: From typical noise floor to max. level for a 1 kHz pure tone signal, A-weighted: 16.6 to 140 dB

Primary Indicator Range: In accordance with IEC 60651, A-weighted: 23.5 dB to 122.3 dB

Linear Operating Range: In accordance with IEC 61672, A-weighted: 1 kHz: 24.8 dB to 139.7 dB

Frequency Analysis

CENTRE FREQUENCIES

1/1-octave Band Centre Frequencies: 63 Hz to 8 kHz

1/3-octave Band Centre Frequencies: 50 Hz to 10 kHz

MEASUREMENTS

L_{ZF} spectrum for display only

L_{Zeq} spectra sampled at 5 ms intervals

MEASURING RANGES

When using Microphone Type 4189:

Dynamic Range: From typical noise floor to max. level for a pure tone signal at 1 kHz 1/3-octave: 1.1 to 140 dB

Linear Operating Range: In accordance with IEC 61260: ≤ 20.5 dB to 140 dB

Internal Generator

Built-in pseudo-random noise generator

Spectrum: Selectable between Pink and White

Crest Factor:

- Pink noise: 4.4 (13 dB)
- White noise: 3.6 (11 dB)

Bandwidth: Follows measurement frequency range

Lower limit: 50 Hz (1/3-oct.) or 63 Hz (oct.),

Upper limit: 10 kHz (1/3-oct.) or 8 kHz (oct.)

Output Level: Independent of bandwidth

Max.: $1V_{rms}$ (0 dB)

Gain Adjustment: –60 to 0 dB

When bandwidth is changed, the level for all bands is automatically adjusted to comply with the set output level

Correction Filters for Sound Sources Type 4292, Type 4295 and Type 4296: Flat or Optimum

Turn-on Time and Turn-off time: Equivalent to RT = 70 ms

Repetition Period: 175 s

Output Connector: Output socket

Control: See Measurement Control

External Generator

Selectable as alternative to internal generator

Controlling external noise generator:

Levels: 0 V (Generator off), 4.5 V (Generator on)

Rise-time and Fall-time: 10 μ s

Control: See Measurement Control

Reverberation Time

EDT, T20 and T30 in octave or 1/3-octave bands

Decays: Measured and stored using averaging time of 5 ms

Evaluation Range: 0 to –10 dB for EDT, –5 to –25 dB for T20 and –5 to –35 dB for T30

Measurement Time: Automatic selection of measurement time for the decays based on the actual reverberation time of the room

Maximum Measurement Time: from 2 to 30 s

Averaging: EDT, T20 and T30 measurements can be averaged (arithmetic averaging or ensemble averaging)

EDT, T20 and T30 Calculation: From slope in evaluation range

Slope Estimation: Least squares approximation

Quality Indicators: Quality indicators with status information like Overload, Curvature in %, etc.; extensive list of status information. Quality indicators are available on reverberation time spectra for each frequency band, and as overall quality indicators for each measurement position and for the total project (room)

Reverberation Time Range: Max. 50 s, min. 0.1 – 0.7 s, depending on bandwidth and centre frequency

Wide Band Reverberation Time: The arithmetic average of the Reverberation Time within a selectable frequency range is calculated

Measurement Displays

OVERVIEW MAP

Map of source and receiver positions with reverberation time readout for a selectable frequency band on each measurement position together with quality indicator.

Organisation of Source and Receiver Positions: Measure at all receiver positions for each source or measure in a number of positions (1 to 10) for each source.

Source and Receiver positions can be added, moved or deleted

OVERVIEW TABLE

Table of measurement positions with reverberation time readout for selectable frequency band on each position together with quality indicator.

Positions can be included/excluded from room average

SOUND LEVEL SPECTRUM

LZF spectrum plus A and C broadband bars

Y-axis: Range: 5, 10, 20, 40, 60, 80, 100, 120, 140 or 160 dB. Autozoom or autoscale available

Cursor: Readout of selected band

Quality indicator for each frequency band

REVERBERATION TIME SPECTRUM

One or two spectra can be displayed

Y-axis: Range: 0.5, 1, 2, 5, 10 or 20 s. Autozoom available

Cursor: Readout of selected band

Quality indicator for each frequency band

REVERBERATION TIME SPECTRUM TABLE

One or two spectra can be displayed in tabular form

DECAY

Decay curve for a position or the room average available for each frequency band

Display of evaluation range and regression line

Readout of Curvature in %

Y-axis: Range: 5, 10, 20, 40, 60, 80, 100, 120, 140 or 160 dB. Autozoom or autoscale available

Measurement Control

Measurement Sequence: Supports measuring:

- at all receiver positions before using another source
- at a receiver position for all sources before measuring at a new position
- at subsequent receiver positions without source information
- at manually selected source and receiver positions

During measurement, the instantaneous sound level spectrum is displayed. After measurement, the reverberation time is displayed

Interrupted Noise Excitation: Measurements are started manually and can be automatically stored on completion of measurement.

The noise generator is turned on and off automatically

Escape Time: 0 to 60 s

Build-up Time: 1 to 10 s

Number of Decays per Measurement: 1 to 100, ensemble averaged into one decay

The generator can be turned on and off manually for checking equipment and sound levels

Serial Measurements:

Selected frequency bands can be measured serially, that is, one by one in an automatic sequence. This can be done automatically in combination with the parallel measurement

Impulse Excitation: Manual start of first measurement. When level (say from starter pistol) exceeds the user-selected trigger level, the decay is

recorded and backwards integration performed (Schroeder method). The trigger can then be armed automatically for measuring at the next position

Signal Recording: Requires license for Signal Recording Option BZ-7226. Recording of the Z-weighted measured signal can be done at each position. For data storage, Signal Recording requires either:

- SD Card
- USB Memory Stick

Measurement Status

ON SCREEN

Information such as *overload*, *awaiting trigger* and *running/paused* are displayed on screen as icons

TRAFFIC LIGHT

Red, yellow and green LEDs show measurement status and instantaneous overload as follows:

- Yellow LED flashing every 5 s = stopped, ready to measure
- Green LED flashing slowly = awaiting trigger or calibration signal
- Green LED on constantly = measuring
- Yellow LED flashing slowly = paused, measurement not stored
- Red LED flashing quickly = intermittent overload, calibration failed

Calibration

Initial calibration is stored for comparison with later calibrations

ACOUSTIC

Using Sound Calibrator Type 4231 or custom calibrator. The calibration process automatically detects the calibration level when Sound Calibrator Type 4231 is used

ELECTRICAL

Uses internally generated electrical signal combined with a typed-in value of microphone sensitivity

CALIBRATION HISTORY

Up to 20 of the last calibrations made are listed and can be viewed on the instrument

Signal Monitoring

Input signal A, C or Z-weighted can be monitored using an earphone/headphones connected to the headphone socket

Headphone Signal: Input signal can be monitored using this socket with headphones/earphones

Gain Adjustment: –60 dB to 60 dB

Annotations

VOICE ANNOTATIONS

Voice annotations can be attached to the reverberation time project, to sources, to receivers and to measurements at each position

Playback: Playback of voice annotations or signal recordings can be listened to using earphone/headphones connected to the headphone socket

Gain Adjustment: –60 dB to 0 dB

TEXT ANNOTATIONS

Text annotations can be attached to the reverberation time project, to sources, to receivers and to measurements at each position

GPS ANNOTATIONS

A text annotation with GPS information can be attached to the project (Latitude, Longitude, Altitude and position error). Requires connection to a GPS receiver

Data Management

Project Template: Defines the display and measurement setups

Project: Measurement data for all positions defined in a room are stored with the Project Template

Job: Projects are organised in jobs

Explorer facilities for easy management of data (copy, cut, paste, delete, rename, view data, open project, create job, set default project name)

User Interface

USERS

Multi-user concept with login. Users can have their own settings with jobs and projects totally independent of other users

PREFERENCES

Date, Time and Number formats can be specified per user

LANGUAGE

User Interface in Catalan, Chinese (People's Republic of China), Chinese (Taiwan), Croatian, Czech, Danish, English, Flemish, French, German, Hungarian, Japanese, Italian, Korean, Polish, Portuguese, Romanian, Russian, Serbian, Slovenian, Spanish, Swedish and Turkish

HELP

Concise context-sensitive help in English, French, German, Italian, Japanese, Korean, Polish, Portuguese, Romanian, Serbian, Slovenian and Spanish

UPDATE OF SOFTWARE

Update to any version (from 4.0 and up) using Measurement Partner Suite BZ-5503 through USB or update via Internet

WEB PAGE

Connect to the analyzer using an Internet browser supporting JavaScript®. The connection is password protected
Two levels of protection:

- Guest level: for viewing only
- Administrator level: for viewing and full control of the analyzer

Specifications – Qualifier Type 7830 and Qualifier Light Type 7831

STANDARDS

All building acoustics standards supported by Type 2250-F/BZ-7227

LANGUAGES

English, French and German

VIEWS

Result Level Views: A collection of views showing the resulting single values, reduction curve and underlying average curves (L1, L2, B2 and T20/T30)

Average Level Views: Each of the parameters (L1, L2 and B2) has a corresponding view showing all of the measurement curves included in the average calculation and a view of the resulting average curve. In T20/T30 Average mode, it is possible to see all of the T20/T30s included in the average calculation. In Ensemble Average mode, it is possible to see the averaged 3D and averaged single frequency decay curves. Both modes gives the user the ability to see the resulting T20/T30 spectrum

Position Level Views: Each of the level measurements (L1, L2 and B2) can be viewed as a spectrum. In addition, the T2 reverberation measurement can be viewed as 3D-multispectra and as single frequency decay curves. Furthermore it is possible to see the calculated T20/T30 spectrum

Data Sheets: All of the measurement and the most relevant intermediate and final results can be viewed as values in a table (not decays)

CURSOR READ-OUT:

All curves have cursor read-out

MANUAL INPUT

Allows graphical input and modification of the regression line in reverberation decay curves. Calculated sound reduction curves can also be adjusted graphically (The impact on the single value index is shown simultaneously). To give maximum flexibility, position, average and calculated data can be overridden by manually inputting data in the data sheets

CALCULATIONS

Supports calculation of insulation and reverberation tasks. Insulation calculations include airborne and impact sound insulation (lab/field). In addition, airborne facade calculation is supported.

REPORT GENERATION

Based on document templates it is possible to make reports conforming to the supported standards

OUTPUT

Relevant views and sheets can be printed or exported to the clipboard. Text or graphs may be transferred to word processors in .rtf (Rich Text Format)

HELP

On-line context-sensitive and user-guide

DATA TRANSFER

- Via RS-232 serial interface: Speeds from 1200 bps to 115200 bps
- Via PC card

MINIMUM PC

- Pentium® III (or newer)
- 256 MB RAM
- SVGA graphics display/adaptor
- Sound card
- CD-ROM drive
- Mouse
- USB
- Serial RS-232 port (to download data directly from the analyzer*)
- PC card slot (for data transfer)
- Windows® XP, Windows Vista® or Windows® 7

* Alternatively, use USB to RS-232 Converter UL-0250

Ordering Information

The ordering information lists the items especially relevant for the Reverberation Time Software. For items related to the Type 2250 platform or other Type 2250 application software, please refer to the Type 2250 Product Data (BP 2025).

Type 2250-F	Hand-held Analyzer with Sound Level Meter and Reverberation Time Software
Type 2250-F-001	Hand-held Analyzer with Sound Level Meter and Reverberation Time Software, Sound Calibrator Type 4231, Qualifier Light Type 7831, 10 m Microphone Extension Cable and Small Tripod
Type 2250-F-002	Hand-held Analyzer with Sound Level Meter, Frequency Analysis, Reverberation Time and Signal Recording Software, Sound Calibrator Type 4231, Qualifier Light Type 7831, 10 m Microphone Extension Cable and Small Tripod

Accessories and Components Available Separately

SOFTWARE MODULES

BZ-7227	2250 Reverberation Time Software
---------	----------------------------------

MEASURING ACCESSORIES

Type 2734-A	Power Amplifier*
Type 2734-B	Power Amplifier with built-in UL-0256 Wireless Audio System*
UL-0256	Wireless Audio System*
Type 4292-L	OmniPower Sound Source*
KE-0449	Flight Case for Type 4292-L*
KE-0364	Tripod Carrying Case for Type 4292-L*
Type 4224	Sound Source
Type 4295	Omnidirectional Sound Source*
KE-0392	Carrying Case for Type 4295*
AO-0523-D-100	Cable from Type 2250 to Power Amplifier, 10 m (33 ft)
AO-0524-D-100	Cable from Type 2250 to Type 4224, 10 m (33 ft)
AQ-0673	Cable from Power Amplifier to Sound Source, 10 m (33 ft)
UA-1476	Wireless Remote Control*

POST-PROCESSING

BZ-5503-A	Measurement Partner Suite, Logging Module†
BZ-5503-B	Measurement Partner Suite, Spectrum Module
Type 7830	Qualifier
Type 7831	Qualifier Light

* For sound source systems and components, please see Product Data [BP 1689](#) or [BP 0066](#)

† For information on the Measurement Partner suite, please see Product Data [BP 2430](#)

TRADEMARKS

Microsoft, Windows, Excel and Windows Vista are registered trademarks of Microsoft Corporation in the United States and/or other countries · Pentium is a registered trademark and Core a trademark of Intel Corporation or its subsidiaries in the United States and/or other countries · JavaScript is a registered trademark of Sun Microsystems Inc.

Brüel & Kjær reserves the right to change specifications and accessories without notice. © Brüel & Kjær. All rights reserved.

HEADQUARTERS: Brüel & Kjær Sound & Vibration Measurement A/S · DK-2850 Nærum · Denmark
Telephone: +45 7741 2000 · Fax: +45 4580 1405 · www.bksv.com · info@bksv.com

Represented in Canada by Xscala Sound & Vibration 403-2747577 info@xscala.com

Brüel & Kjær 

